





FIG. .

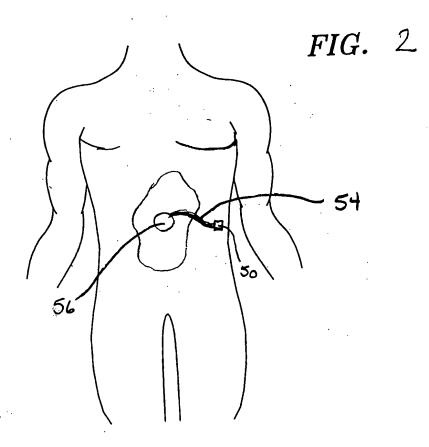


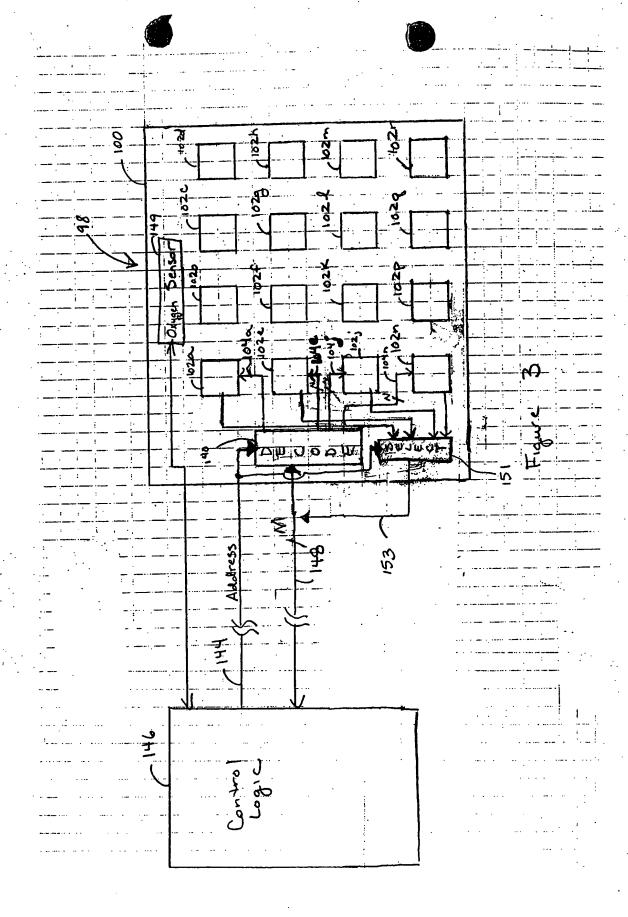

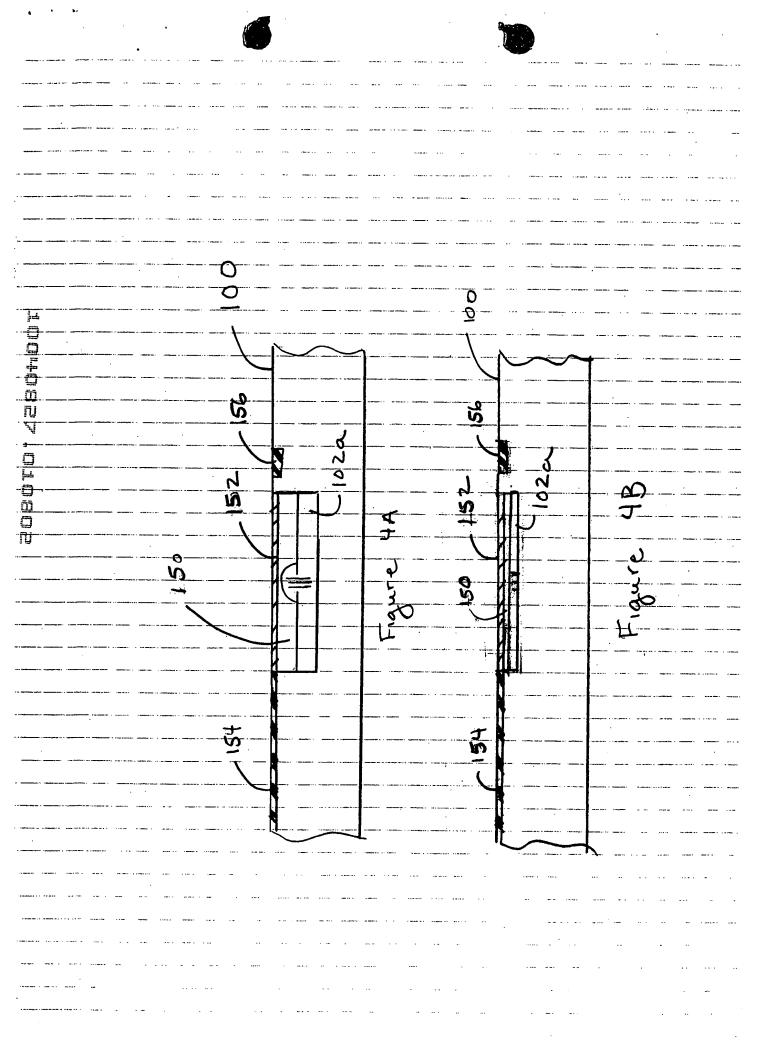

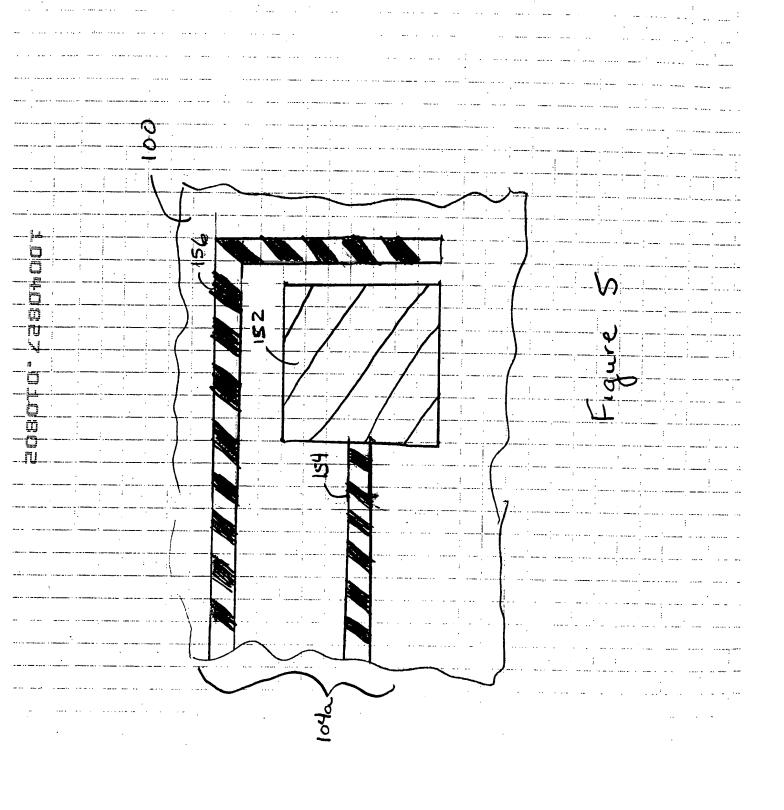

...

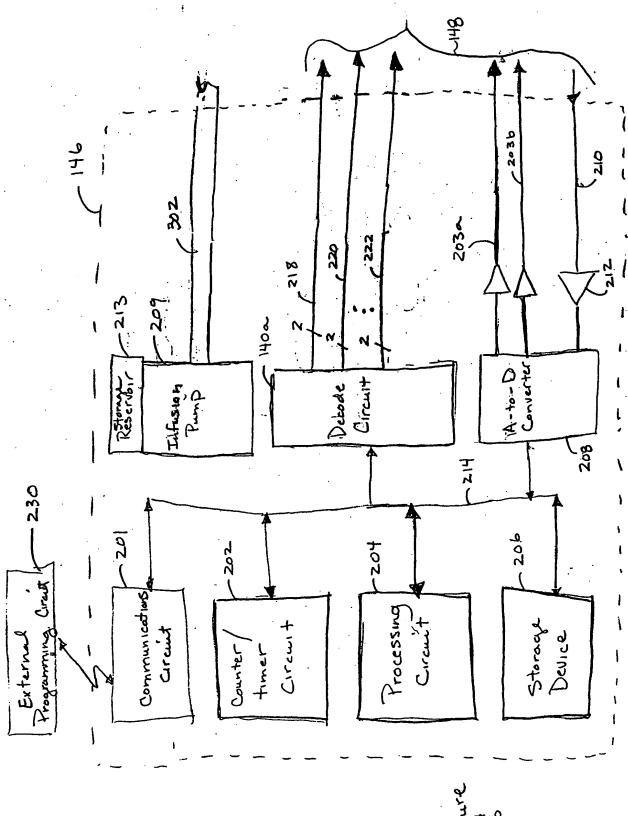

Haure

	300
Activate one on me array by dissolving protection	thue member formed of procompatible, bioCompatible material (metal, endiblege)
Calibrate activated	5ensors
	/304
Obtain measure activated Sen	ments from one or more sors (e.g. time-multiplexed transfer
	30x
Perform desired Pi using averaging, data proc	rocessing of sensor data. Voting, andor any other essing brethods
	308
Adjust therapy store result to external user and sensor	based on Sensor data, s transfer data system, notify for otherwise willize data
	370
If any Sensor an out-of-ran replacemen	data is approaching ge condition, activate sensors
	312
No - All Sen	fors are activated?
Va .	4769
-+	- User
Do	1314 ne